

Quik-ID® Class I

INTENDED USE

Quik-ID® Class I is a qualitative solid phase enzyme linked immunosorbent assay (ELISA) designed to detect Panel Reactive IgG antibodies (PRA) to HLA class I antigens.

For *In Vitro* Diagnostic Use.

SUMMARY AND EXPLANATION

HLA is a major antigenic system in determining the survival of transplant allografts or transfused platelets in sensitized individuals.¹ HLA antibodies can be acquired through alloimmunization as a result of pregnancy, transfusion of blood products, or previous transplants. In general, alloimmunization leads to the production of HLA antibodies in approximately 33% of exposed individuals.²

The highly polymorphic human leukocyte (HLA) class I antigens are widely distributed on all nucleated cells. Platelets, although not nucleated, are fragments of nucleated megakaryocytes and carry the class I antigens.³

Quik-ID® Class I Solid Phase ELISA provides HLA class I glycoproteins derived from the platelets or EBV transformed B lymphocyte cell lines of 40 donors, each immobilized in different microwells by means of a monoclonal antibody. The HLA class I type of each donor and the number of wells containing each antigen can be found on the Recording Sheet.

Quik-ID® Class I Solid Phase ELISA is designed to be used as a companion product to QUIKSCREEN®. Samples previously identified as positive in the screening assay can be further tested on Quik-ID® Class I to determine a PRA value and/or specificity.

PRINCIPLES OF THE PROCEDURE

Patient serum is added to microwells coated with HLA class I glycoproteins allowing antibody, if present, to bind. Unbound antibodies are then washed away. An alkaline phosphatase labeled anti-human globulin reagent (Anti-IgG) is added to the wells and incubated. The unbound Anti-IgG is washed away and the substrate PNPP (p-nitrophenyl phosphate) is added. After a 30-minute incubation period, the reaction is stopped by a sodium hydroxide solution. The optical density of the color that develops is measured in a spectrophotometer.

REAGENTS

Maximum number of tests per kit: 10

All reagents should be stored as directed by the label.

- | | |
|------------|--|
| MS | 1. Microwells: Flat-bottom microwell strips to which HLA class I glycoproteins have been immobilized. The microwell strips are color coded and enclosed in resealable foil pouches. Ready for use. |
| TCW | 2. Concentrated Wash (10x): Tris (hydroxymethyl) aminomethane buffered solution containing sodium chloride and Tween 20. 1% sodium azide. Dilute with deionized or distilled water before use. Store Working Wash solution up to 48 hours at room temperature or up to seven days at 2 to 8°C. |
| SD | 3. Specimen Diluent: Phosphate buffered saline solution containing bovine albumin and mouse serum. 0.1% sodium azide. Ready for use. |
| SB | 4. Substrate Buffer: This solution contains diethanolamine and magnesium chloride. 0.02% sodium azide. Ready for use. Protect from light. |
| SS | 5. Stopping Solution: 3 M Sodium Hydroxide. Ready for use. Use with care. |

- | | |
|-----------|--|
| AG | 6. Conjugate: Alkaline phosphatase conjugated goat affinity purified antibody to human immunoglobulin G (IgG). 0.1% sodium azide. Dilute in Specimen Diluent before use. |
| PN | 7. PNPP (p-nitrophenyl phosphate) Substrate: Crystalline powder. Reconstitute with deionized or distilled water and dilute in Substrate Buffer before use. Protect from light. |
| PC | 8. Positive Serum Control: Human Serum. 0.1% sodium azide. Dilute in Specimen Diluent before use. |
| NC | 9. Negative Serum Control: Human Serum. 0.1% sodium azide. Dilute in Specimen Diluent before use. |
| PS | 10. Plate Sealers. |

PRECAUTIONS

- Do not use reagents that are turbid or contaminated.
- Care **MUST** be taken to avoid contamination of Specimen Diluent and Conjugate. Inadvertent contamination of these reagents with human serum will result in the neutralization of the Conjugate and subsequently to test failure.
- Do not use reagents beyond their expiration date.
- Microwells and reagents contained in the kit are not to be used in conjunction with any other test system.
- Substitution of components other than those provided in this kit may lead to inconsistent or erroneous results.
- Discard any unused portions of diluted Conjugate, diluted Positive and Negative Controls, and diluted and reconstituted PNPP reagent after each run.
- When making dilutions, follow pipet manufacturer's instructions for appropriate dispensing and rinsing techniques.
- The enzyme substrate reaction which occurs in the final incubation is temperature sensitive and should be performed in a controlled area at 22 to 25°C.
- Due to variations in instruments or consistently higher or lower room temperatures, it may be necessary for the laboratory to establish a slightly longer or shorter incubation time in order to consistently achieve valid control results. Because the temperature of the final incubation can affect control values, it is important to periodically monitor the room temperature incubation.

CAUTION

- All human serum used in the Positive and Negative controls for this product has been tested and found negative for antibody to HIV, HCV and HBsAg by FDA approved methods. No test method, however, can offer complete assurance that HIV, Hepatitis C virus, Hepatitis B virus or other infectious agents are absent. Therefore, these materials should be handled as potentially infectious.
- Some of the reagents supplied with this kit contain sodium azide as a preservative.
WARNING: Sodium azide reacts with lead and copper plumbing forming highly explosive metal azides. When discarded in a sink, the sink should be flushed with a large volume of water to prevent azide buildup. Sodium azide is a poison and is toxic if ingested.
- Stopping Solution (NaOH) is corrosive. Avoid contact with skin and eyes. Spills should be cleaned up immediately.
- Discard all components when completed according to local regulations.

SPECIMEN COLLECTION

Blood should be collected without anticoagulant using aseptic technique and should be tested while still fresh to minimize the chance of obtaining false positive or false negative reactions due to improper storage or contamination of the specimen. Samples that cannot be tested immediately should be stored at 2 to 8°C for no longer than 48 hours or frozen. Samples frozen at -20°C or below remain in good condition for several years (2-3 years). However, in order to avoid the deleterious effect of repeated freeze/thaw cycles, it is recommended that samples should be aliquoted in small volumes and then stored frozen. Avoid frost-free freezers.

Serum should be separated from red cells when stored or shipped.

Particulates or aggregates in the sample can cause false positive results or poor duplicate values. Samples containing particulate matter should be clarified by centrifugation prior to testing.

Only whole human serum is suitable for this assay. Prior dilution of samples in anything other than normal, ELISA negative human serum could affect the results.

Microbially contaminated, hemolyzed, lipemic, icteric, or heat inactivated samples may give inconsistent results and should be avoided.

PROCEDURE

Materials Provided:

Vials may contain more reagent than described on the labels. Be sure to measure the reagent with an appropriate device when making dilutions.

1. 5 Microwell frames, each containing 12 - 1 x 8 color coded strips and a color key card
2. 1 x 125 mL Concentrated Wash
3. 1 x 50 mL Specimen Diluent
4. 1 x 60 mL Substrate Buffer
5. 1 x 50 mL Stopping Solution
6. 1 x 350 μ L Anti-Human IgG Conjugate
7. 5 x 50 mg PNPP Substrate
8. 1 x 0.3 mL Positive Serum Control
9. 1 x 0.7 mL Negative Serum Control
10. 10 Plate Sealers

Additional Materials Required:

1. Test tubes for patient sample and control dilutions and for reagent dilutions
2. Transfer pipets
3. Adjustable micropipets to deliver 10 – 100 μ L and 100 – 1,000 μ L and disposable tips
4. Timer
5. Microplate reader capable of measuring OD at 405 or 410 and 490 nm
6. Deionized or distilled water
7. Absorbent paper towels
8. Microplate washer or device
9. Centrifuge capable of separating serum or plasma from patient samples
10. 37°C waterbath or incubator

Test Procedure

1. Bring all reagents to room temperature.
2. Make Working Wash solution by diluting Concentrated Wash. Add 1 volume of Concentrated Wash to 9 volumes of deionized or distilled water. Mix well.

Reagent	1 Plate (2 Samples)	2 Plates (4 Samples)	3 Plates (6 Samples)	4 Plates (8 Samples)	5 Plates (10 Samples)
TCW	28 mL	53 mL	78 mL	103 mL	125 mL
DI Water	252 mL	477 mL	702 mL	927 mL	1,125 mL

3. Determine the number of patient samples to be tested.

PREPARE SAMPLES AND CONTROLS

4. Dilute as follows and mix well:

Patient Sample	550 μL
SD	1.650 mL

Reagent	1 Plate (2 Samples)	2 Plates (4 Samples)	3 Plates (6 Samples)	4 Plates (8 Samples)	5 Plates (10 Samples)
NC	150 μL	250 μL	350 μL	450 μL	550 μL
SD	450 μL	750 μL	1,050 μL	1.35 mL	1.65 mL
PC	35 μL	60 μL	85 μL	115 μL	135 μL
SD	105 μL	180 μL	255 μL	345 μL	405 μL

5. Each sample requires one set of color-coded strips. Promptly remove and reseal the unneeded strips in the protective pouch.

NOTE: Orient the frame with A1 in the top left corner. Be sure that all strips are properly seated and snapped into their frame. Label or number each strip to avoid errors. Maintain the same plate orientation throughout the assay.


Ensure that the rounded tab on each strip is at the bottom edge of the frame. Before each reagent addition, ensure that well A1 is in the top left-hand corner of the frame.

NOTE: Be sure that the order of the strips in the frame matches the order on the color key card.

6. Add 250 μL of Working Wash solution to all wells and allow to stand at room temperature for 5-10 minutes.

7. Aspirate or decant forcefully and invert on absorbent toweling to prevent drying.

8. Add 50 μL of the appropriate diluted control or sample to the wells as designated in figure 1. Add patient serum to all numbered wells and to the NA well.

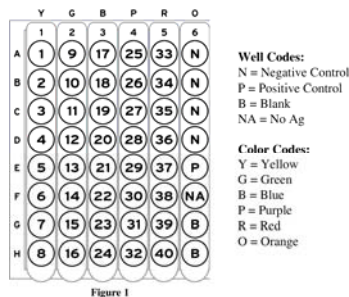

NOTE: Do not add samples or reagents to blank wells.

NOTE: If multiple patient samples are tested at the same time, LABEL EACH STRIP TO AVOID ERRORS.

9. Seal the microwells with a plate sealer and incubate for 30-35 minutes in a 37°C waterbath. If a dry incubator is used instead, increase time by 10 minutes.

10. Dilute the Conjugate 1 to 100 in Specimen Diluent. Use a polypropylene container.

Reagent	1 Plate (2 Samples)	2 Plates (4 Samples)	3 Plates (6 Samples)	4 Plates (8 Samples)	5 Plates (10 Samples)
AG	50 μL	100 μL	150 μL	200 μL	250 μL
SD	5 mL	10 mL	15 mL	20 mL	25 mL

NOTE: Conjugate is viscous. Prime tip 2-3 times in Conjugate before dispensing and rinse after addition to Specimen Diluent. Mix well.

11. WASH STEP

- a) Aspirate or decant contents of each well and blot on absorbent toweling.
- b) Add 250 μL Working Wash solution.
- c) Aspirate or decant.
- d) Repeat steps b + c for a total of 3 or 4 washes.
- e) Vigorously decant to remove all residual wash solution. Invert on absorbent toweling to prevent drying.

NOTE: It is important to completely remove all wash solution after the final wash.

12. Add 50 μL of diluted Conjugate (made in a previous step) to all wells EXCEPT those designated as BLANKS.
13. Seal the microwells with a plate sealer and incubate for 30-35 minutes in a 37°C waterbath. If a dry incubator is used instead, increase time by 10 minutes.
14. Dissolve PNPP Substrate by adding 0.5 mL deionized or distilled water to the vial. Replace stopper and mix well. Protect from light until use.
15. Dilute the PNPP 1 to 100 in the Substrate Buffer.

Reagent	1 Plate (2 Samples)	2 Plates (4 Samples)	3 Plates (6 Samples)	4 Plates (8 Samples)	5 Plates (10 Samples)
PN	100 μL	200 μL	300 μL	400 μL	500 μL
SB	10 mL	20 mL	30 mL	40 mL	50 mL

Mix well. Protect from light until use.

16. WASH STEP:

- a) Aspirate or decant contents of each well and blot on absorbent toweling.
- b) Add 250 μL Working Wash solution.
- c) Aspirate or decant.
- d) Repeat steps b + c for a total of 3 or 4 washes.
- e) Vigorously decant to remove all residual wash solution. Invert on absorbent toweling to prevent drying.

Proceed promptly through next three steps.

17. Add 100 μL of the diluted PNPP solution to all the wells EXCEPT those designated as BLANKS.
18. Allow the microwells to stand in the dark for 30 minutes at ROOM TEMPERATURE (22 to 25°C).

NOTE: Incubation time and temperature after the addition of PNPP is critical. DO NOT vary the established incubation time or temperature. For consistency, begin timing promptly after addition of the reagent to the first well.

19. Stop the reaction by adding 100 μL of Stopping Solution to each well in the same sequence as the addition of the substrate. Add 200 μL of Stopping Solution to the blank wells.
20. Read the absorbance (OD) of each well at 405 or 410 nm using a reference filter of 490 nm. If the results cannot be read immediately, return the wells to a dark location for up to 30 minutes.
21. Subtract the values obtained in the blank wells from all sample and control wells. Many ELISA readers are programmed to automatically perform this step.
22. Record the results on the Recording Sheet.

QUALITY CONTROL

Quality control of Quik-ID® Class I is built into the test system by the inclusion of Positive and Negative Serum Controls. These controls should be included with each test sample to help determine if technical errors or reagent failures have occurred. Criteria for a valid test:

	Negative Control	Positive Control
Mean OD	≤ 0.250	≥ 1.200

INTERPRETATION OF TEST RESULTS

Calculate the Cutoff value for each individual well as follows:

$$\begin{array}{l} \text{Mean of Neg. Control wells} \\ \text{(A, B, C, \& D of Orange strip)} \end{array} \times 2 \times \begin{array}{l} \text{Background Adjustment Factor} \\ \text{(see Recording Sheet)} \end{array} = \begin{array}{l} \text{Cutoff Value} \\ \text{for the well} \end{array}$$

Test results showing OD values equal to or greater than the cutoff value are regarded as being positive results. Calculate the % PRA as follows:

$$\% \text{ PRA} = \frac{\# \text{ of Positive Results}}{\# \text{ of wells containing HLA class I antigen}} \times 100$$

LIMITATIONS

Erroneous results can occur from bacterial contamination of test materials, inadequate incubation periods, inadequate washing or decanting of test wells, exposure of substrate to stray light, omission of test reagents, exposure to higher or lower than prescribed temperature requirements, or omission of steps.

The presence of immune complexes or other immunoglobulin aggregates in the patient sample may cause an increased non-specific binding and produce false-positives in this assay.

The results of this assay should not be used as the sole basis for a clinical decision.

Some low titer, low avidity antibodies may not be detected using this assay.

The No Antigen Well (well F of orange strip) does not contain monoclonal antibody or HLA glycoproteins and is used to detect non-specific binding.

Patient samples that give higher values in the "No Antigen Well" than the cutoff value of the negative control should be tested by another method.

Non-HLA lymphocytotoxic antibodies will not be detected using this assay.

This product does not detect IgM, IgA, or HLA class II antibodies.

Some non-cytotoxic HLA antibodies may be detected by this technique that do not react in the lymphocytotoxicity assay (LCA).

This product is expected to detect HLA antibodies to antigens that are represented on the panel (see lot specific Recording Sheet). Antibodies to unrepresented antigens may not be detected.

SPECIFIC PERFORMANCE CHARACTERISTICS

When properly stored and used according to the procedures described above, this product can detect antibodies to the HLA class I antigens identified on the enclosed Recording Sheet.

To ensure suitable reactivity and specificity, each lot of Quik-ID[®] Class I is tested prior to release with samples known to contain alloantibodies reactive with HLA class I antigens as well as samples known to be free of such antibodies.

Performance Evaluation

		Comparative Method		Total
		Positive	Negative	
Quik-ID [®] Class I	Positive	14	0	14
	Negative	0	7	7
	Total	14	7	21

Agreement: 100%

Co-positivity: 100% Co-negativity: 100%

Comparative Method: ELISA method for PRA Determination

REFERENCES

1. Marsh SGE, Parham P, Barber LD, The HLA Facts Book. Academic Press 2000: 84-91.
2. Rodey Glenn E. HLA Beyond Tears. De Novo, Inc. 2000; 213.
3. Harrison J, Navarrete C., Selection of Platelet Donors and Provision of HLA Matched Platelets, in Histocompatibility Testing. Imperial College Press, 2000; 379.
4. Zachary AA, Delaney NC, Lucas DP, Laffell MS. Characterization of HLA Class I Specific Antibodies by ELISA Using Solubilized Antigen Targets: I. Evaluation of the GTI Quik-ID Assay and Analysis of Antibody Patterns. Human Immunology 2001; 62:3, 228-235.

U.S. Patent #6,046,013



GTi DIAGNOSTICS[®]
 Good science starts with people.[®]

20925 Crossroads Circle, Suite 200
 Waukesha, WI 53186-4054 USA
 (262) 754-1000 OR 1-800-233-1843

Quik-ID[®] Class I

- FOR *IN VITRO* DIAGNOSTIC USE
- STORE AT 2 to 8°C



Cat. NO. QID
 Rev. 12 March 2008



Qarad b.v.b.a.
 Volmolenheide 13
 B-2400 Mol
 Belgium

www.gtidiagnostics.com